

# INFECTION CONTROL AND HOSPITAL EPIDEMIOLOGY<sup>®</sup>

## EDITORIAL

- Classification of the Surgical Wound: A Time for Reassessment  
and Simplification 253  
RONALD LEE NICHOLS, MD

## ORIGINAL ARTICLES

- Validation of Surgical Wound Classification in the Operating Room 255  
DENISE M. CARDO, MD; PAMELA S. FALK, MPH; C. GLEN MAYHALL, MD
- Oxacillin- and Quinolone-Resistant *Staphylococcus aureus* in Sao Paulo,  
Brazil: A Multicenter Molecular Epidemiology Study 260  
HELIO S. SADER, MD; ANTONIO C. PIGNATARI, MD; RICHARD J. HOLLIS, MS; IVANI LEME, MS;  
RONALD N. JONES, MD
- A Cluster of Surgical Wound Infections due to Unrelated Strains of Group A  
Streptococci 265  
E.B. JAMIESON, MD, FRCPC; K. GREEN, RN, CIC; D.E. LOW, MD, FRCPC  
A.E. SIMOR, MD, FRCPC; C. GOLDMAN, BSCN; J. NG, ART; A. MCGEER, MD, FRCPC
- Brucellosis Among Hospital Employees in Saudi Arabia 268  
FRANK W. KIEL, MD; M. YOUSUF KHAN, MD

## READERS' FORUM

- Wash Hands, Disinfect Hands, or Don't Touch? Which, When, and Why? 273  
ALLAN PERCEVAL, MSC, MASM

## PRODUCT COMMENTARY

- Efficacy of Chemical Sterilants/Disinfectants: Is There a Light at the End  
of the Tunnel? 276  
INGE GUREVICH, RN, MA

## BEYOND INFECTION CONTROL: THE NEW HOSPITAL EPIDEMIOLOGY

- Agency for Healthcare Policy and Research 279  
BRYAN P. SIMMONS, MD; STEPHEN B. KRITCHEVSKY, PHD

## TOPICS IN CLINICAL MICROBIOLOGY

- Rhodococcus* 282  
ROBERT D. WALSK, MD, PHD; PAUL E. SCHOCH, PHD; BURKE A. CUNHA, MD

## LETTERS TO THE EDITOR


- Cost Improvement Through Prudent Infection Control in a Brazilian Hospital 250  
HEIKO GEISS, MD

- Universal Precautions Kit 252  
PHYLLIS A. KEPHART, MD; KATHLEEN L. ROMAN, RN, BSN-ICN; DEBORAH M. MYERS

- MEDICAL NEWS 289

- SHEA NEWS 299

# Dream Machine.

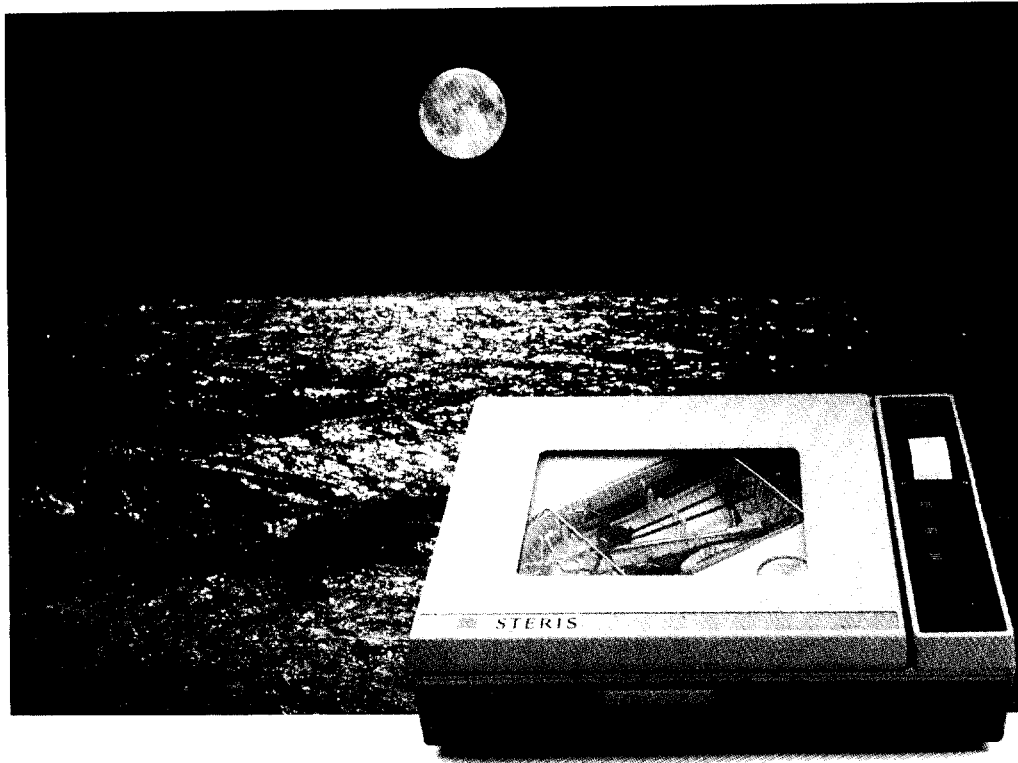

**Rapid, Safe,  
Sterile Processing  
Was Once  
Just A Dream**

● STERIS SYSTEM 1™ has made the dream of rapid and safe sterile processing a reality.

STERIS SYSTEM 1 is the proven, low temperature sterile processing system for immersible surgical and diagnostic devices. Even delicate, heat sensitive scopes, cameras, instruments, and accessories can be safely sterilized in less than 30 minutes-Just In Time for each patient procedure. ●

STERIS SYSTEM 1 also provides peace of mind. There are no toxic fumes, and no disposal restrictions to lose sleep over. ● And liquid processing means that your devices can be sterilized without the drying and wrapping which are required with gaseous systems.

Write or call us today to learn why thousands of health professionals rest assured with the rapid and safe sterile processing of STERIS SYSTEM 1. ○

**The STERIS PROCESS™  
The Proven Process  
Just In Time**

**STERIS®**



# Answers To Commonly Asked Questions About the STERIS PROCESS™

## LIQUID STERILE PROCESSING

Q. How does liquid sterile processing compare to other methods? Q. How is the STERIS PROCESS different from other liquid processes?

A. Regardless of the sterilization process, the item to be sterilized must be clean to ensure effective sterilization. The cleaning process is universally performed by washing an item with water. Gas sterilization technologies, such as EtO and vaporized hydrogen peroxide, require that an item be completely dry before it is exposed to the sterilization process. This adds time, difficulty, and uncertainty—all negatives when a health professional is rushing to get ready to treat the next patient.

Since the STERIS PROCESS uses a liquid sterilant, it is equally effective on wet or dry items. This allows processing of items immediately after pre-cleaning without additional preparation. And since the STERIS PROCESS does not require wrapping and unwrapping of items, it eliminates many processing steps which are typically performed with gaseous systems, and allows sterilization with optimum efficiency and efficacy.

Liquid processing offers many other advantages as well. Liquid solutions are more easily directed than gases. This is especially important when processing sophisticated devices such as lumened endoscopes, which pose a challenge to chemical sterilization technologies. In addition, sterile processing with STERIS SYSTEM 1™ allows the user to see the gentle agitation of the liquid solution in action, without having to rely on complex monitoring systems to ensure that the sterilizing agents are present.

A. The STERIS PROCESS uses STERIS 20™, a powerful chemical sterilant with a high degree of materials compatibility. The STERIS 20 formulation includes the active biocidal agent, peracetic acid, in combination with a proven chemical protection system. The ability to deliver anti-corrosives to all surfaces of a device is an important advantage of a liquid system.

The STERIS PROCESS is used in STERIS SYSTEM 1—a complete sterile processing system. SYSTEM 1 provides automated and documented sterile processing in less than 30 minutes, so sterile devices are available Just In Time for each patient procedure.

Q. How is the STERIS 20 solution different from other solutions, like glutaraldehyde?

A. Glutaraldehyde solutions are typically used only to disinfect, not sterilize. These solutions are normally reused, allowing contamination and/or dilution. Unlike STERIS 20, glutaraldehyde cross links proteins, and therefore, can affix organic material to instrument surfaces. The STERIS 20 formulation, along with the directed flow of SYSTEM 1, makes the STERIS PROCESS more effective at reaching contaminated surfaces.

STERIS 20 does not have the same hazardous waste and worker exposure considerations as glutaraldehyde. The STERIS 20 use dilution is non-toxic and safely disposed in an ordinary drain during the standard processing cycle. In fact, it has passed the stringent fish toxicity tests required by the U.S. EPA and the State of California.

---

STERIS Corporation develops, manufactures, and markets sterile processing and infection prevention systems for the worldwide healthcare market. STERIS® is committed to providing products which improve patient and worker safety. If you would like more information about STERIS or STERIS SYSTEM 1, please write or call us at 1-800-JIT-4-USE (1-800-548-4873).

Paid Advertisement





# **VACUTAINER<sup>®</sup> BRAND** **Safety-Lok<sup>™</sup>** **BLOOD COLLECTION SET**

## **Ease of use**

because safety and ease of use  
are built into the design.



## **Ease of mind...**

because your focus  
should be on your patient



For use in accordance with the  
OSHA Bloodborne Pathogens Standards.  
Please refer to package insert for  
caution statement before use.

For more information, please call  
**1-800-631-0174.**

**BECTON  
DICKINSON**

Becton Dickinson VACUTAINER Systems, Franklin Lakes, New Jersey 07417-1885  
VACUTAINER and Safety-Lok are trademarks of Becton Dickinson and Company.  
US Patent Number 5,120,320

© 1993

**Meets OSHA guidelines:  
Engineered for safety  
New**

# INFECTION CONTROL AND HOSPITAL EPIDEMIOLOGY<sup>TM</sup>

## CONTENTS

### EDITORIAL

- Classification of the Surgical Wound: A Time for Reassessment and Simplification 253  
RONALD LEE NICHOLS, MD

### ORIGINAL ARTICLES

- Validation of Surgical Wound Classification in the Operating Room 255  
DENISE M. CARDO, MD; PAMELA S. FALK, MPH; C. GLEN MAYHALL, MD
- Oxacillin- and Quinolone-Resistant *Staphylococcus aureus* in Sao Paulo, Brazil: A Multicenter Molecular Epidemiology Study 260  
HELIO S. SADER, MD; ANTONIO C. PIGNATARI, MD; RICHARD J. HOLLIS, MS; IVANI LEME, MS; RONALD N. JONES, MD
- A Cluster of Surgical Wound Infections due to Unrelated Strains of Group A Streptococci 265  
E.B. JAMIESON, MD, FRCPC; K. GREEN, RN, CIC; D.E. LOW, MD, FRCPC; A.E. SIMOR, MD, FRCPC; C. GOLDMAN, BSCN; J. NG, ART; A. MCGREER, MD, FRCPC
- Brucellosis Among Hospital Employees in Saudi Arabia 268  
FRANK W. KIEL, MD; M. YOUSUF KHAN, MD

### READERS' FORUM

- Wash Hands, Disinfect Hands, or Don't Touch? Which, When, and Why? 273  
ALLAN PERCEVAL, MSc, MASM

### PRODUCT COMMENTARY

- Efficacy of Chemical Sterilants/Disinfectants: Is There a Light at the End of the Tunnel? 276  
INGE GUREVICH, RN, MA

### BEYOND INFECTION CONTROL: THE NEW HOSPITAL EPIDEMIOLOGY

- Agency for Healthcare Policy and Research 279  
BRYAN P. SIMMONS, MD; STEPHEN B. KRITCHEVSKY, PHD

### TOPICS IN CLINICAL MICROBIOLOGY

- Rhodococcus* 282  
ROBERT D. WALSH, MD, PhD; PAUL E. SCHOCH, PhD; BURKE A. CUNHA, MD

### DEPARTMENTS

- Letters to the Editor 250
- Medical News 289
- Calendar of Events 296
- SHEA News 299

THE PUBLICATION OF ADVERTISING IN THE JOURNAL DOES NOT CONSTITUTE ANY GUARANTEE OR ENDORSEMENT BY THE SOCIETY FOR HOSPITAL EPIDEMIOLOGY OF AMERICA OR SLACK INCORPORATED OF THE ADVERTISED PRODUCT OR SERVICE OR OF CLAIMS MADE BY THE ADVERTISER. THE PUBLICATION OF ARTICLES AND OTHER EDITORIAL MATERIAL IN THE JOURNAL DOES NOT NECESSARILY REPRESENT THE POLICY RECOMMENDATIONS OR ENDORSEMENT BY THE SOCIETY.

**PUBLISHER:** Infection Control and Hospital Epidemiology (ISSN-0899-823X, Canadian GST#129780466) is published exclusively by SLACK Incorporated 12 times a year. Address: 6900 Grove Rd., Thorofare, NJ 08086. Telephone: (609) 848-1000.

**COPYRIGHT 1993** The Society for Hospital Epidemiology of America, Inc., and SLACK Incorporated. All rights reserved. No part of this publication may be reproduced without written permission from the publisher. Printed in the USA.

**SUBSCRIPTIONS:** Requests should be addressed to the publisher (except Japan). In Japan, contact Woodbell Incorporated, 4-22-11, Kitakasai, Edogawaku, Tokyo 134, Japan. Subscription rates in the United States and possessions: Individual: One year-\$80.00; Two years-\$115.00; Three years-\$145.00; Institutional: One year-\$90.00; Two year-\$130.00; Three years-\$170.00. Fellows: \$20 per year with proof of training status. Canada: \$18.00 additional each year plus 7% for Canadian Goods & Services tax; all other countries: \$36.00 additional each year. Single copies of current issues may be obtained for \$15.00, United States and possessions; \$20.00 all other countries.

**REPRINTS:** All requests to reprint or use material published herein should be addressed to Lester Robeson, SLACK Incorporated, 6900 Grove Rd., Thorofare, NJ 08086. For reprint orders and prices, contact Lester Robeson at (609) 848-1000. Authorization to photocopy items for internal or personal use, or the internal or personal use of specific clients, is granted by SLACK Incorporated, provided that the base fee of \$1.00 per copy, plus \$15 per page is paid directly to Copyright Clearance Center, 27 Congress St., Salem, MA 01970. This consent does not extend to other kinds of copying, such as for general distribution, resale, advertising and promotional purposes, or for creating new collective works.

**CHANGE OF ADDRESS:** Notice should be sent to the publisher six weeks in advance of effective date. Include old and new addresses with zip codes. The publisher cannot accept responsibility for undelivered copies. Second-class postage is paid at Thorofare, New Jersey 08086, and additional entry points. **POSTMASTER:** Send address changes to SLACK Incorporated, 6900 Grove Rd., Thorofare, NJ 08086.

INFECTION CONTROL AND HOSPITAL EPIDEMIOLOGY is listed in Index Medicus, Current Contents—Clinical Practice, Hospital Literature Index, Cumulative Index to Nursing & Allied Health Literature, Nursing Abstracts, and Laboratory Performance Information Exchange System.



## EDITORIAL OFFICES

Vanderbilt University School of Medicine  
A-1131 Medical Center North  
Nashville, TN 37232-2637  
(615) 343-1095; (615) 343-1882 (FAX)  
Email: [iche@mcmail.vanderbilt.edu](mailto:iche@mcmail.vanderbilt.edu)

## EDITOR

Michael D. Decker, MD, MPH

## MANAGING EDITOR

Susan Cantrell

## STATISTICAL EDITOR

Beverly G. Mellen, PhD

## SENIOR ASSOCIATE EDITORS

C. Glen Mayhall, MD

Gina Pugliese, RN, MS

William Schaffner, MD

## ASSOCIATE EDITORS

Donald A. Goldmann, MD

Didier Pittet, MD, MS

Andreas Widmer, MD, MS

## SECTION EDITORS

### Beyond Infection Control:

#### The New Hospital Epidemiology

Bryan P. Simmons, MD

Stephen B. Kritchevsky, PhD

Memphis, Tennessee

Wing Hong Seto, MD

Hong Kong

### Disinfection and Sterilization

William A. Rutala, PhD, MPH

Chapel Hill, North Carolina

### Emerging Infectious Diseases

Larry J. Strausbaugh, MD

Portland, Oregon

Robert W. Pinner, MD

Atlanta, Georgia

### From the Laboratory

Marcus Zervos, MD

Royal Oak, Michigan

Fred C. Tenover, PhD

Atlanta, Georgia

### Information Management

John A. Sellick, DO

Buffalo, New York

### The International Perspective

Mary D. Nettleman, MD, MS

Richmond, Virginia

### Issues in Surgery

James T. Lee, MD, PhD

St. Paul, Minnesota

### Medical News

Gina Pugliese, RN, MS

Chicago, Illinois

Martin S. Favero, PhD

Irvine, California

### Practical Healthcare Epidemiology

Loreen A. Herwaldt, MD

Iowa City, Iowa

### SHEA News

Murray D. Batt, MD

Clarksburg, West Virginia

### Statistics for Hospital Epidemiology

David Birnbaum, PhD, MPH

Sidney, British Columbia, Canada

### Topics in Long-Term Care

Philip W. Smith, MD

Omaha, Nebraska

### Topics in Occupational Medicine

David Weber, MD, MPH

Chapel Hill, North Carolina

# INFECTION CONTROL AND HOSPITAL EPIDEMIOLOGY®

## EDITORIAL ADVISORY BOARD

Jacques F. Acar, MD	Paris, France
J. Wesley Alexander, MD	Cincinnati, Ohio
Paul Arnow, MD	Chicago, Illinois
Graham A.J. Ayliffe, MD	Birmingham, United Kingdom
Neil L. Barg, MD	Yakima, Washington
Elizabeth Ann Bolyard, RN, MPH, CIC	Atlanta, Georgia
John M. Boyce, MD	Providence, Rhode Island
Professor Dr. Ilja Braveny	Munich, Federal Republic of Germany
Charles Bryan, MD	Columbia, South Carolina
Christian Brun-Buisson, MD	Creteil, France
Donald E. Craven, MD	Boston, Massachusetts
Sue Crow, MSN, RN, CIC	Shreveport, Louisiana
Franz Daschner, MD	Freiburg, Federal Republic of Germany
Leigh G. Donowitz, MD	Charlottesville, Virginia
Charles E. Edmiston, Jr., PhD	Milwaukee, Wisconsin
Theodore C. Eickhoff, MD	Denver, Colorado
Bruce Farber, MD	Manhasset, New York
Victoria J. Fraser, MD	St. Louis, Missouri
Peter C. Fuchs, MD, PhD	Black Butte, Oregon
Richard A. Garibaldi, MD	Farmington, Connecticut
Velvl Greene, PhD, MPH	Beer Sheva, Israel
Robert Gaynes, MD	Atlanta, Georgia
David W. Gregory, MD	Nashville, Tennessee
David K. Henderson, MD	Bethesda, Maryland
Peter N.R. Heseltine, MD	Los Angeles, California
Karen Hoffmann, RN, CIC, MS	Chapel Hill, North Carolina
Marguerite McMillan Jackson, RN, PhD	San Diego, California
Janine Jagger, MPH, PhD	Charlottesville, Virginia
William R. Jarvis, MD	Atlanta, Georgia
Douglas S. Kernodle, MD	Nashville, Tennessee
Robert H. Latham, MD	Nashville, Tennessee
Lewis B. Lefkowitz, MD	Nashville, Tennessee
Hsieh-Shong Leu, MD, MSc	Taipei, Taiwan
Jack Levy, MD	Brussels, Belgium
Victor Lorian, MD	Bronx, New York
Dennis G. Maki, MD	Madison, Wisconsin
Professor Dr. Walter Marget	Munich, Federal Republic of Germany
William J. Martone, MD	Bethesda, Maryland
Allison McGeer, MD	Toronto, Ontario, Canada
John E. McGowan, Jr., MD	Atlanta, Georgia
Jonathan L. Meakins, MD, DSc	Montreal, Quebec, Canada
Raf Mertens, MD	Brussels, Belgium
Robert R. Muder, MD	Pittsburgh, Pennsylvania
Joseph M. Mylotte, MD, CIC	Buffalo, New York
Lindsay Nicolle, MD	Winnipeg, Manitoba, Canada
Juhani Ojajarvi, MD	Helsinki, Finland
Michael T. Osterholm, PhD, MPH	Minneapolis, Minnesota
Jan Evans Patterson, MD	San Antonio, Texas
Sindy M. Paul, MD	Trenton, New Jersey
Michael A. Pfaller, MD	Iowa City, Iowa
Samuel Ponce de Leon, MD, MSc	Mexico City, Mexico
Isaam Raad, MD	Houston, Texas
Manfred L. Rotter, MD, DipBact	Vienna, Austria
Theodore Sacks, MD	Jerusalem, Israel
William E. Scheckler, MD	Madison, Wisconsin
Kent Sepkowitz, MD	New York City, New York
Denis Spelman, MD	Prahran Victoria, Australia
Michael L. Tapper, MD	New York, New York
Clyde Thornsberry, PhD	Brentwood, Tennessee
Professor Leonid P. Titov	Minsk, Republic of Belarus
Timothy R. Townsend, MD	Millwood, Virginia
Antoni Trilla, MD, PhD	Barcelona, Spain
Professor Wang Shu-Qun	Beijing, People's Republic of China
J. John Weems, Jr., MD	Greenville, South Carolina
Robert A. Weinstein, MD	Chicago, Illinois
Professor Dr. W. Weuffen	Greifswald, Federal Republic of Germany
Sergio B. Wey, MD	São Paulo, Brazil
Rebecca Wurtz, MD	Evanston, Illinois

## SLACK Incorporated

6900 Grove Road  
Thorofare, New Jersey 08086  
(609) 848-1000

### Vice President/Group Publisher

Richard N. Roash

### Publisher

John C. Carter

### Editorial Director

Jennifer Kilpatrick

### Production Editor

Shirley P. Strunk, ELS

### Assistant Editor

Eileen C. Anderer

### Circulation Manager

Lester J. Robeson, CCCP

### Production Director

Christine Malin

### Production Coordinator

Joanne Patterson

### Publishing Director/ Advertising

Wayne McCourt

### Pharmaceutical Group Sales Director

Michael LoPresti

### Advertising Sales Representative

Jennine Kane

### Classified/Recruitment Sales Manager

Michele Burch

# What do you mean I'm *not* protected?

If you are in the habit of applying hand cream after using a Chlorhexidine Cluconate (CHC) handwash, you may actually be losing your protection! A recent study\* confirms that residual CHC can be neutralized by anionic hand creams.

Introducing.. **Lotion Soft@ Skin Conditioner**, a nonionic skin care lotion compatible with any CHG handwashing product. **Lotion Soft@ Skin Conditioner** contains emollients and moisturizers, which are soothing and last through several handwashes.

When you scrub with CHC for antimicrobial protection, you should be using a compatible product for skin conditioning. Try new **Lotion Soft@ Skin Conditioner**. It will not interfere with the cumulative effects of CHG.

Contact your local Calgon Vestal Healthcare Market Specialist or call toll-free 1-800-325-8005 to find out about new CHG compatible **Lotion Soft@ Skin Conditioner**.

**Lotion Soft Skin Conditioner**  
*The compatible companion*



DIVISION OF CALGON CORPORATION  
SUBSIDIARY OF **MERCK**  
& CO., INC.

Box 147, ST. LOUIS, MO 63166

**1-800-325-8005**

See us at Booth "A" APIC

*\*test data on file*