

INDEX TO ADVERTISERS	
Diatome	Cover 3, A10
EDAX	A8, A11
Electron Microscopy Sciences, EMS	Cover 2, A7
Hitachi	Cover 4, A9
Panasonic i-Pro	A4





Competitive Performance, Compact Package—The FlexSEM 1000 II VP-SEM

The Hitachi FlexSEM 1000 II Scanning Electron Microscope features big power in a small package with the highest in-class resolution of 4.0 nm, user-friendly operation, and many automated functions that enable high-quality data acquisition for beginners to experts alike. With integrated space saving technology, the FlexSEM 1000 II allows users to have the capabilities of a full-sized SEM in a compact, efficient package.














Polymers

3-D & CLEM

Materials





Electronics

Biology




Contact Us for a Virtual Demonstration at hta-microscopy@hitachi-hightech.com

Hitachi High-Tech America, Inc.

www.hitachi-hightech.com/us hta-microscopy@hitachi-hightech.com $\begin{array}{l} Tel (800-253-3053) \\ \text{https://doi.org/10.1017/5143192/821013787} \end{array} \\ \text{Published online by Cambridge University Press} \\ \end{array}$ Hitachi Social Innovation is

POWERING GOOD

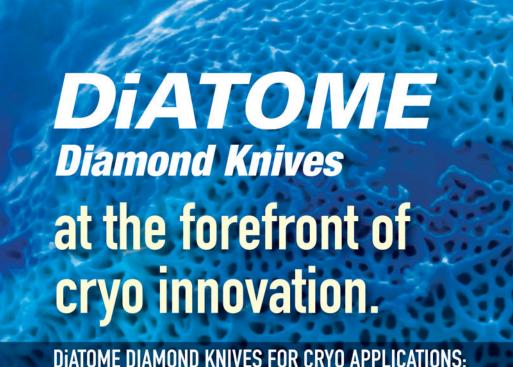

cryo immuno

The first cryo knife with a diamond platform, guarantees the best possible sectioning for cryo-immuno-chemistry.





trimtool 20, 45, and 90

One trimming tool for all of your trimming needs, be it at room or cryo temperatures.



P.O. Box 410 • 1560 Industry Rd. Hatfield, Pa 19440

Tel: (215) 412-8390 • Fax: (215) 412-8450 email: info@diatomeknives.com

Please visit our website for our complete range of Diamond Knives.

www.diatomeknives.com





Available for wet or dry sectioning.




histo cryo

Available as boats for wet cryo sectioning, and triangular holders for dry cryo sectioning. Made of a special copper/nickel alloy, which guarantees the best heat/cold transmission.


cryo AFM

Specially tested to ensure that they meet the increased quality requirements of AFM investigation.



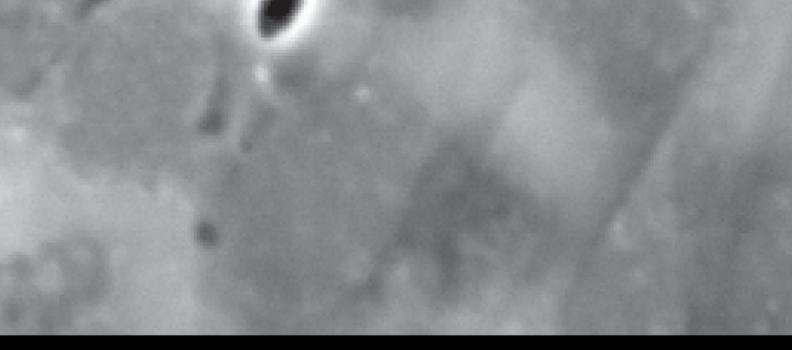

Recharge Your Lithium Research

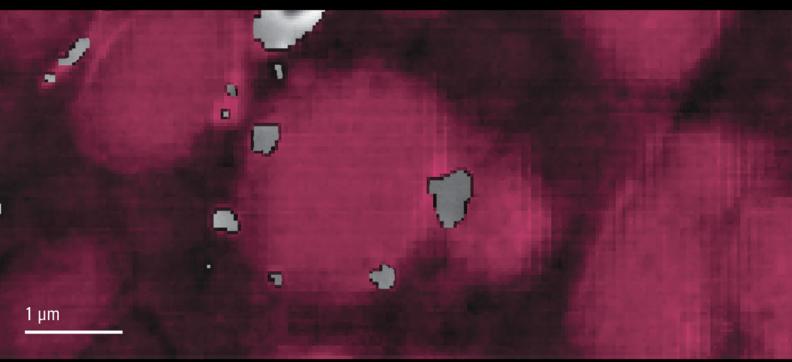



Enabling quantitative mapping of lithium in the SEM

For the first time, lithium distribution in a lightweight MgLiAl structural alloy is mapped in the scanning electron microscope. Using the Octane Elite Super (EDAX) and OnPoint™ (Gatan) detectors, the composition by difference method was used to reveal the distribution of single-digit mass percentages of lithium quantitatively across the macro-, micro- and nano-scales. See www.gatan.com/lithium for the full experiment brief.

AMETEK®



DIATOME

the incomparable Diamond Knife for all fields of research...

Jeknives

DiATOME Diamond Knives are the premier knife for biological and materials applications, compatible with all

For decades, researchers have relied on DiATOME Diamond Knives superior quality, reliability, and durability. And with proper use, they require far less resharpening than any other knife, making them economical as well.

Resharpened DiATOME knives undergo the same stringent optical checking and sectioning test as new knives. The same flawless quality is quaranteed.

Applications are numerous and include sectioning of hard or soft industrial samples, embedded biological samples, alternating ultrathin/semithin, and frozen hydrated samples. Please see our website for a complete applications guide.

Get them from **THE** source...

DIATOME U.S.

P.O. Box 410 • 1560 Industry Rd. Hatfield, Pa 19440

Tel: (215) 412-8390

Fax: (215) 412-8450

email: info@diatomeknives.com

NEUROSCIENCE

Micro-Optical Sectioning Tomography to Obtain a High-Resolution Atlas of the Mouse Brain Anan Li, Hui Gong, Bin Zhang, Qingdi Wang, Cheng Yan, Jingpeng Wu, Qian Liu, Shaoqun Zeng, Qingming Luo

Britton Chance Center for Biomedical Photonics, Wuhan National Laboratory for Optoelectronics—Huazhong University of Science and Technology, Wuhan 430074, P. R. China.

CRYO


A single slice of a tomogram of an aldehyde fixed and sucrose infiltrated cryosection with a 3D reconstruction. Erik Bos and Peter J. Peters, Netherlands Cancer Institute, Amsterdam. (see: J. Lefman, P. Zhang, T. Hirai, RM. Weis, J. Juliani, D. Bliss, M. Kessel, E. Bos, P.J. Peters, S. Subramaniam: Three-dimensional electron microscopic imaging of membrane invaginations in Echerichia coli overproducing the chemotaxis receptor Tsr. J. Bacteriol. 2004 Aug; 186(15): 5052-61.)



MATERIALS

ABS, stained with OsO₄, sectioned at room temperature with the ultra sonic knife, section thickness 50nm. Note the almost perfect spherical shape of the large rubber particles and the preservation of the inclusions inside. Also the smaller dense rubber particles are well preserved. B.Vastenhout, Dow Benelux N.V. Terneuzen, The Netherlands.










Cutting-Edge Applications Require Cutting-Edge Instrumentation

Today's rapidly evolving applications require superior imaging, high throughput, and reliable runtime. Hitachi, the award-winning innovator in Field-Emission SEM, offers a broad range of options for semiconductor, materials, and life science applications. Explore the Hitachi EM portfolio and maximize your analyses with platforms designed for users of all experience levels as well as many configurations to fit your needs and budget.

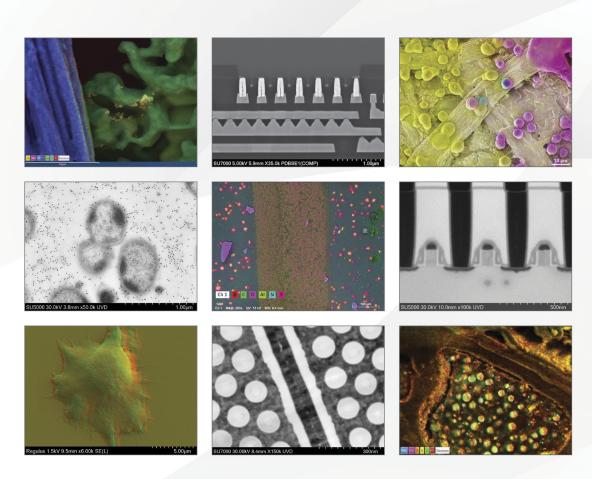

Request a Virtual Demonstration

@Hitachi High-Tech America, Inc.

www.hitachi-hightech.com/us
hta-microscopy@hitachi-hightech.com
Tel. 800-253-3053
https://doi.org/10.1017/5143192/621013787 Published online by Cambridge University Press

Hitachi Social Innovation is

POWERING GOOD