

X-ray Diffraction Reference Standards and Zero-background Sample Plates Custom Designed and Built for any Application

Your first step to improved x-ray
diffraction results should be to
contact The Gem Dugout for quality
diffraction alignment standards and
zero-background plates.
And the next step is successful
x-ray diffraction results.

The Gem Dugout
1652 Princeton Drive
State College, PA 16803
(814) 865-5782

Capillary Tubes and Laboratory Supplies for X-Ray Diffraction Use

Kodak Direct Exposure Film especially developed for X-ray diffraction analysis. Available in 35mm x 20m rolls and in 50 sheet boxes.

Polaroid XR-7 High Speed X-Ray Diffraction Cassettes for Laue and Precession Photography, and Polaroid 3000 Speed Film, Type 57, in single-exposure packets.



CAPILLARY TUBES

Special Glass and Quartz in 15 sizes from 0.1mm to 3.5mm O.D. Uniform 89mm length and funnel shaped at the top. 0.01mm wall thickness.

Manufacturers of Fine
X-Ray Diffraction Equip-
ment For Over 45 Years

Charles Supper Company
INCORPORATED

15 TECH CIRCLE, NATICK, MA 01760, U.S.A.
TELEPHONE: (508) 655-4610 PD21
1-800-323-9645

Attend an ICDD Short Course & Workshop



Advance your PDF Skills

- Learn to identify/characterize crystalline substances using powder diffraction data.
- Build proficiency in interpretation of experimental powder data – especially using the *Powder Diffraction File*.
- Hands on work sessions ... manual & computer search methods ... comprehensive work book provided.

April 1991

Florida

For further information contact:
 Ms. Josephine Felizzi
 JCPDS-ICDD
 1601 Park Lane, Swarthmore, PA 19081
 USA (215) 328-9400 Telex: 847170

PD22




EISI

Elemental and Interplanar Spacing Index

Utilizing experimental d-Spacings and elemental data ...

Search using combinations of Elemental Data Compound Formulae and then ...

Identify matches EISILY



Now available

for ED
for XRD

International Centre for Diffraction Data
 1601 Park Lane, Swarthmore, PA 19081 U.S.A.
 (215) 328-9400 Telex: 847170 Fax: (215) 328-2503

PD23

Supplier Source Directory

Tell the powder diffraction community about . . .
 your services, catalogs, new products, excess equipment
 in the Supplier Source Directory.

Low Cost.


Easy to use.

Business card format.

Powder Diffraction announces the Supplier Source Directory – designed for use by those who wish to make known their special services to the X-ray diffraction community. Rates are modest (no discounts for agencies), beginning at \$125.00 for one insertion (business card size).

For details please write or call Mary M. Rossi, Advertising Manager, JCPDS-ICDD at Swarthmore. (215-328-9403).

Macintosh Search/Retrieval Software for the PDF-2 Database



Helios Software, Inc.

Charles E. Rose
 P.O. Box 44-1215
 W. Somerville, MA 02144

Tel. 802-785-2042

Advertisers in Powder Diffraction December 1990 Volume 5 Number 4

Company	Page Number	PD Number
Charles Supper Company	VII	PD7
Charles Supper Company	XVII	PD21
Dapple Systems	XIV	PD16
Enraf Nonius	IX	PD10
Fein-Marquart Associates	XIII	PD15
Gem Dugout	XVII	PD20
inel Instrumentation Electronique	IV	PD4
Ital Structures	VIII	PD9
ICDD - EISI	XVIII	PD23
ICDD - For 1990/91	XIV	PD17
ICDD - PC-PDF CD-ROM	XV	PD18
ICDD - Schools	XVIII	PD22
ICDD - Set 35-36	X	PD12
Materials Data, Inc.	X	PD11
Philips	Back Cover	PD25
PICXAM	XII	PD14
Radix Instruments	VI	PD6
Rigaku, U.S.A.	Inside Back Cover	PD24
Scintag, Inc.	V	PD5
Seifert X-Ray Corporation	XVI	PD19
Siemens	Inside Front Cover	PD1
Siemens	I	PD2
Sietronics Pty. Ltd.	XI	PD13
SPEX	II	PD3
Steuerungstechnik	VII	PD8

Powder Diffraction Reader Reply Card — Volume 5, Number 4, Dec. 1990

Advertiser's Information: Circle Number

PD1	PD2	PD3	PD4	PD5	PD6	PD7	PD8	PD9	PD10
PD11	PD12	PD13	PD14	PD15	PD16	PD17	PD18	PD19	PD20
PD21	PD22	PD23	PD24	PD25	PD26	PD27	PD28		

JCPDS-ICDD Information: Check to Receive Information

<input type="checkbox"/> APD Type Data Base	<input type="checkbox"/> Book Form X-ray Data	<input type="checkbox"/> CD-ROM
<input type="checkbox"/> Common Phases Search Manual	<input type="checkbox"/> Educational Packages	<input type="checkbox"/> EISI Index
<input type="checkbox"/> Electron Diffraction Search/Match	<input type="checkbox"/> Microcomputer Search/Match	
<input type="checkbox"/> Microfiche Package	<input type="checkbox"/> NIST Crystal Data	<input type="checkbox"/> Short Courses

Name/Title _____

Institution Company _____

Phone _____

Address _____

City _____ State _____ Zip _____

Country _____ Mail Code _____

Please enter my subscription for

Credit Cards now accepted

Powder Diffraction

Annual subscription rate: 1990

- U.S. & Canada \$45.00 (U.S. dollars)
- Library Rate \$85.00 (U.S. dollars)
- Far East Rate Write Sanyo Information System Corp., Taiyo Bldg. 7-7, Tomizawa-cho Nihonbashi, Chuo-ku, Tokyo 103, Japan for subscriptions for Japan, China, Taiwan, Malaysia, the Philippines, Indonesia and Korea.

Other annual subscriptions: 1990

- \$65.00 (U.S. dollars)
- Library Rate
- \$85.00 (U.S. dollars)

Type of subscription:

- Academic
- Government
- Manufacturing
- Personal
- Other

Name/Title _____

Institution/Company _____

Address _____

Phone _____

City _____ State _____ Zip _____

Country _____ Mail Code _____

Charge: Visa MasterCard Signature _____

Number _____ Exp. Date _____

Please enter my subscription for

Credit Cards now accepted

Powder Diffraction

Annual subscription rate: 1990

- U.S. & Canada \$45.00 (U.S. dollars)
- Library Rate \$85.00 (U.S. dollars)
- Far East Rate Write Sanyo Information System Corp., Taiyo Bldg. 7-7, Tomizawa-cho Nihonbashi, Chuo-ku, Tokyo 103, Japan for subscriptions for Japan, China, Taiwan, Malaysia, the Philippines, Indonesia and Korea.

Other annual subscriptions: 1990

- \$65.00 (U.S. dollars)
- Library Rate
- \$85.00 (U.S. dollars)

Type of subscription:

- Academic
- Government
- Manufacturing
- Personal
- Other

Name/Title _____

Institution/Company _____

Address _____

Phone _____

City _____ State _____ Zip _____

Country _____ Mail Code _____

Charge: Visa MasterCard Signature _____

Number _____ Exp. Date _____

TRUE MICRO DIFFRACTION

IN 3-D

Down to 11 μm Dia. or 5 μg Quantity

X-ray diffraction analysis of extremely small areas or extremely small samples can now be done with ease with the Rigaku PSPC/MDG. Three axis (ω , χ and ϕ) sample oscillation solves the problem of spotty patterns from only a few crystal grains of micro samples. The curved position sensitive detector allows simultaneous measurement of a 2θ range of 0 to 150 degrees. This minimizes the time required for data collection and produces high detection sensitivities for micro samples. A few highlights:


- 3 axis (ω , χ and ϕ) oscillation
- Simultaneous 0 to 150 degrees data collection
- Easy sample alignment
- Selection of x-ray sources
- Selection of computer processing
- Motorized X-Y-Z sliding stage (optional)
- 35 mm camera kit (optional)
- TV camera for remote viewing (optional)
- Can be added to an existing x-ray diffraction unit

Rigaku's expertise in the design and manufacture of x-ray sources and accessories is unsurpassed. For more information — give us a call !


X-ray... our only business !

Rigaku

Rigaku/USA, Inc., Northwoods Business Park, 200 Rosewood Dr., Danvers, MA 01923
Phone (508) 777-2446 ■ FAX (508) 777-3594

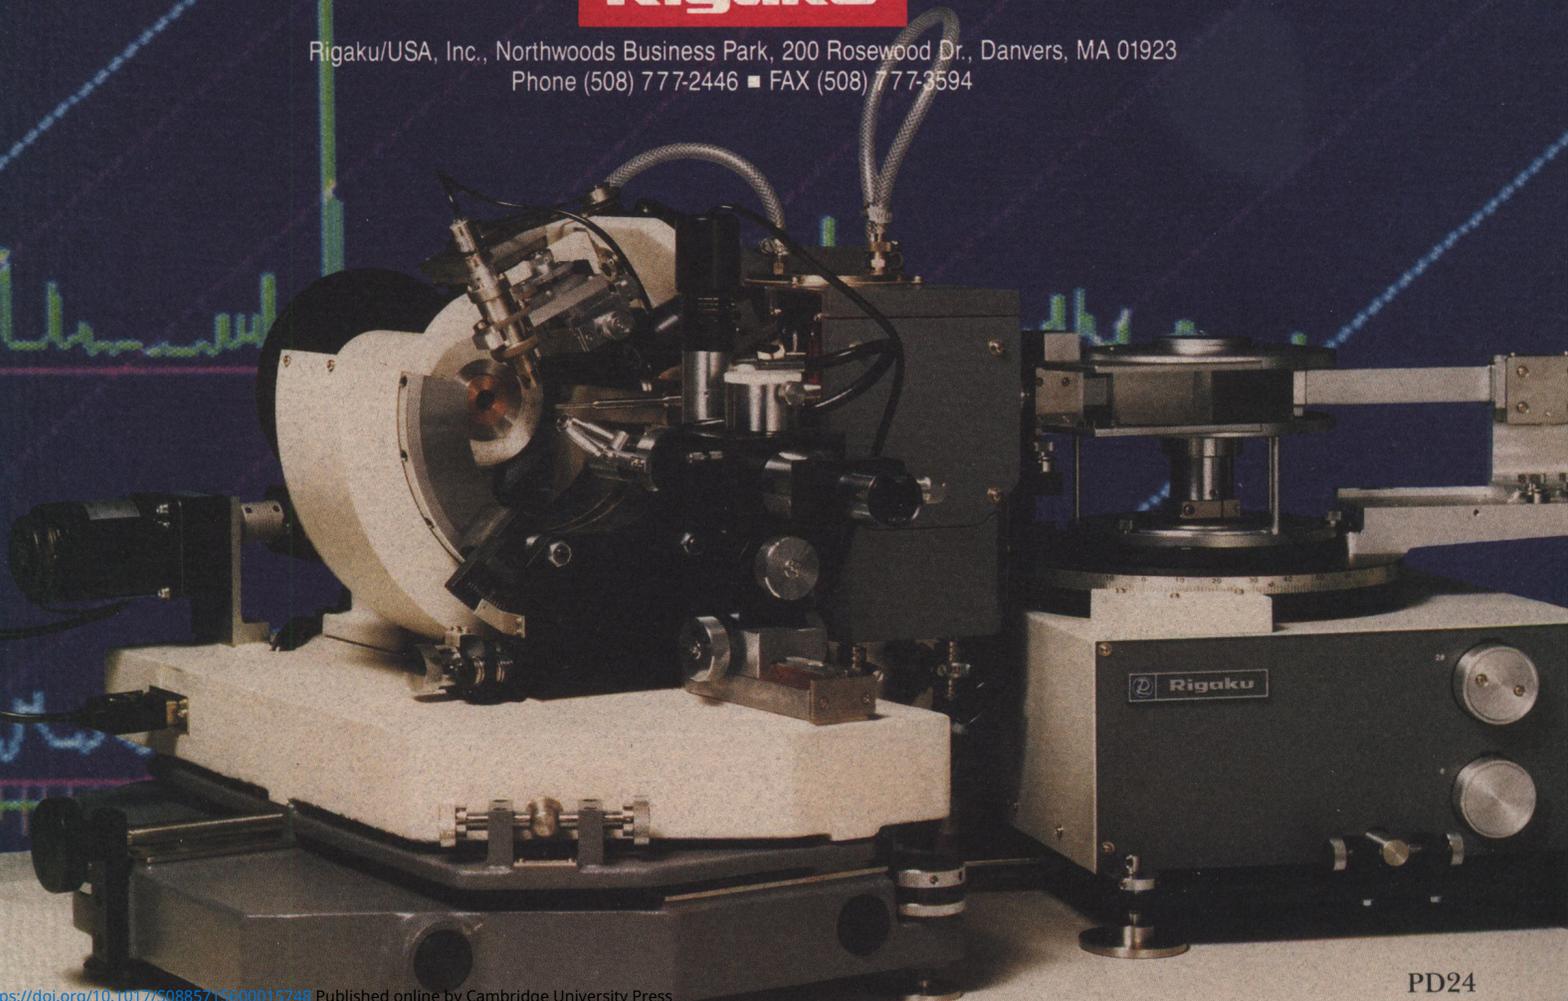

From now on all other powder diffractometers will be measured against this one.

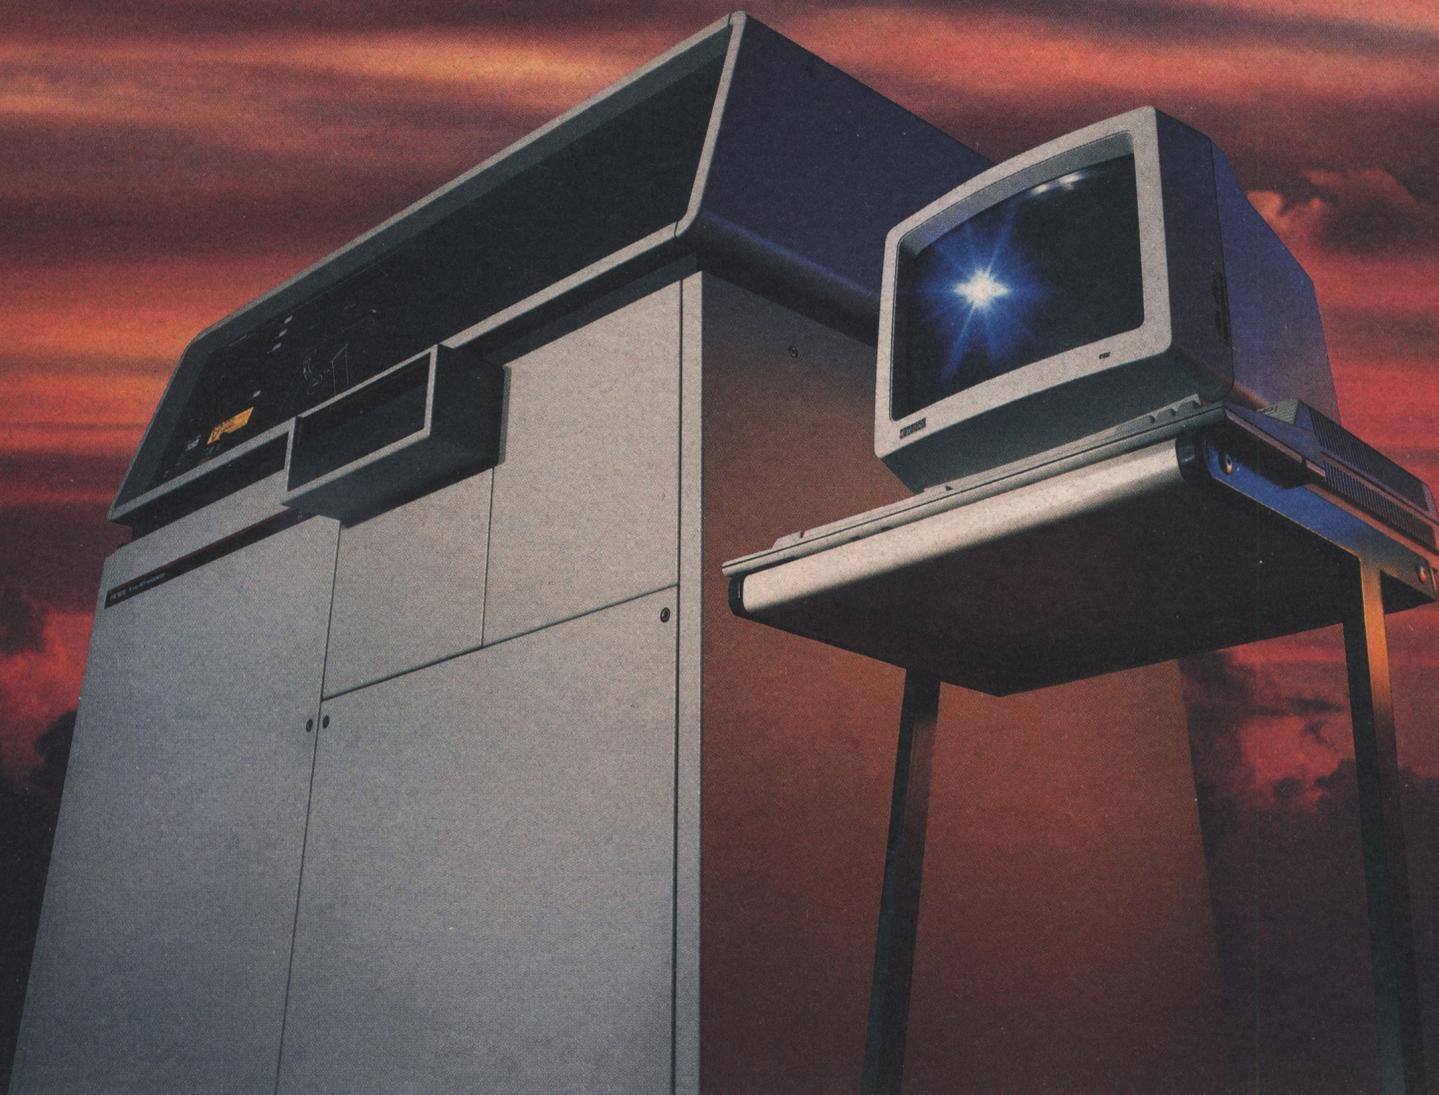

It's the new Philips PW1800.

It's the most advanced system of its type available anywhere. It's also the most versatile and the easiest to operate.

It's designed for easy, automatic measurement of a wide range of sample types in a variety of forms and quantities including powders, clays, pastes and filters. Built-in electronics control and supervise all diffractometry functions to assure reliability. What's more, the PW1800 actually monitors itself to see that it is functioning properly. And alerts the operator if it senses trouble ahead. In fact, everything about this new system has been engineered to simplify operation.

Even its appearance underscores its uniqueness. It's totally enclosed, totally integrated to assure complete radiation and contamination protection. Which means it can be installed safely and quickly in the laboratory or on the production line.

And among the things you don't see in this unique system is the newly developed, permanently-aligned goniometer that combines ease of operation with high precision and outstanding analytical performance. Built-in robotics for sample handling. And a new, highly-efficient generator that not only requires less space, but actually reduces power consumption as well.

It's the new Philips PW1800. It's the new standard of the industry. And it's backed by the worldwide support resources of the Philips organization.

For complete details, contact:

Philips Electronic Instruments, Analytical X-Ray Group,
85 McKee Drive, Mahwah, NJ 07430, Tel. (201) 529-3800.

(Outside U.S.A.) Philips Scientific & Analytical Equipment,
Industrial & Electro-acoustic Systems, Lelyweg 1,
7602 EA Almelo, The Netherlands. Tel (31) 5490-39911.



PHILIPS

PD25