CrossMark


In biology and biomedicine, optical microscopy has rapidly progressed from the simple observation of static cellular and sub-cellular components to increasingly complex studies of the interrelationships of structure, function and local biochemical environment (pH, Ca⁺⁺concentration, etc.). Low noise CCD cameras have been critical in this ongoing evolution. Originally used merely to capture two dimensional low light images (fluorescence, absorption or Raman), these cameras are now being used to generate a variety of multidimensional data. These other dimensions may include spectral information, temporal (time resolved) information and more recently, the third spatial dimension.

In this article, we examine a newly commercialized technique, called digital image restoration microscopy, that utilizes a high performance CCD camera to generate quantitative images.

The principles involved are fairly simple. The CCD camera is used to record a series of two dimensional (x,y) images at different depths (z) in a fluorescently labelled sample. This is performed by sequentially moving the focal plane of the microscope. The resultant image "slices" are then mathematically combined to create a full three dimensional image. This can be displayed on the system monitor, either as slices, or as a 3-D rendering, which can be rotated for viewing from any angle.

Of course, when the microscope is focused on a particular plane in the object, the CCD camera is also receiving out of focus light from outside this plane. The trick to producing well focused final images is to deal with this out of focus light in some way.

In confocal laser scanning microscopes (CLSMs), out of plane light is simply eliminated by spatial filtering with a confocal pinhole. Such a system is optically inefficient because so much of the light is discarded. For this reason, samples must be treated with large concentrations of fluorophores.

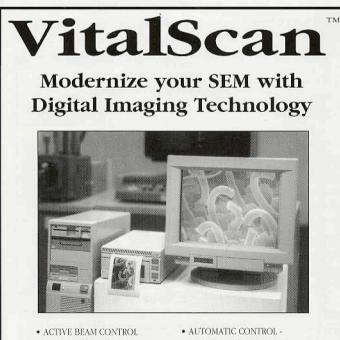

- ACTIVE BEAM CONTROL
 UP TO 4096x4096 CAPTURE
- (12-BIT Digitization)DUAL ADC'S (Collect Secondary)
- and Backscatter) • FRAME and PIXEL AVERAGING
- AUTOMATIC CONTROL -CONTRAST/BRIGHTNESS
 OPTIONAL FAST X-RAY
- MAPPING
- OPTIONAL IMAGE ANALYSIS
 SOFTWARE

Vital Image Technology • 800-860-IMAGE

Vital Image Technology offers photographic-quality printers and other imaging related products such as CCD cameras, frame grabbers and scanners. VIT has the imaging solution for both network and stand alone applications. In digital image restoration microscopy, a conventional lamp source is used for illumination, and all the fluorescent light from the sample is collected. Computer algorithms then "reassign" locations for out of focus photons to produce a sharp image. The algorithms are empirically fitted to the individual microscope's optical performance during a simple training phase. Basically, a fluorescent bead, smaller that the microscope's optical resolution, is placed on the sample stage. In focus and out of focus images are recorded so that the software learns how the microscope's optics transform this light. In normal imaging operation, this so-called point spread function is then used by the system to reassign all out of focus photons to their correct *xyz* points of origin.

This technique has been known in the research community for over 15 years, being pioneered by groups at the University of Massachusetts and the University of California (San Francisco). The proven techniques and algorithms developed by these researchers have been licensed and developed into commercial instruments by Scanalytics (Billerica, MA), Applied Precision, Inc. (Mercer Island, WA), and VayTeck, Inc. (Fairfield, IA), using Photometrics CCD cameras. Although their instruments differ in details of both hardware and software, they are similar in that each consists of a cooled CCD camera coupled to a research grade optical microscope. In all, the CCD is interfaced to a powerful microprocessor; the sample is flat-field illuminated by use of a filament lamp and fiber bundle.

How do these instruments compare to CLSMs? According to Carl Brown of Applied Precision, "For biologists involved with *in vivo* studies, this technique is much less disruptive than a CLSM." First lower levels of fluorescent indicators and labels are required, because of the high optical efficiency of the microscope. Also, the cells are not subject to the heating and photobleaching effects of a tightly focused laser beam. Even with low intensity illumination, the images can be accumulated and stored very rapidly (a few seconds). As a consequence, dynamic processes can be studied in 3-D over extended periods of time. The refocusing of the photons, referred to as exhaustive photo reassignment, or EPR[™] by Scanalytics, takes from a few minutes to tens of minutes depending on the hardware platform and the size of the image.

In terms of spatial resolution, these instruments are capable of 0.25 μm resolution in the *xy* plane and 0.6 μm resolution in the *z* direction, which is certainly better than a CLSM even under optimal conditions. Summarizes Scanalytics' David Hitrys, "This technique allows us to breach what is typically thought of as the diffraction limit for light based microscopy."

So why has it taken so long for commercial products to emerge? Both companies are in agreement that it is the recent availability of CCD cameras combining low noise with high speed, together with affordable microcomputers with the power to run the "focusing" algorithms. States Hitrys, "Another benefit of our instrument is that the final reconstructed fluorescent image is quantitative, and can even be used for ratio imaging. In order to achieve this, a 12-bit dynamic range is an absolute minimum requirement."

Applied Precision's DeltaVision uses a Photometrics *PXL*[™] with a Kodak (KAF 1400) CCD array. They chose *PXL*[™] because its SCSI interface works directly with their SGI workstation. Adds Brown, "The KAF 1400 chip is virtually ideal because of its small, densely packed pixels, which translates directly into high spatial resolution." In terms of physical size, the KAF 1400 array also matches well with the central "flat field" portion of the microscope's image plane. Only this central region is used, because the refocusing algorithms are not quite as effective at the outside edges of the microscope's field of view.

To demonstrate the power of this technique, the figure shows images of a NRK (normal rat kidney) containing a Rhodamine label for the protein tubulin. The left image is a typical XY slice recorded by the CCD, and the right image is after processing.

In conclusion, all companies predict that the combined benefit of 3-D information, high spatial resolution, and minimal *in vivo* disruption will lead to rapid growth of this technique, now that turnkey commercial instruments are readily available.

Reprinted from Photometrics CCD Newsbrief, summer, 1994.



MICROSCOPY MICROANALYSIS KANSAS CITY, AUG. 13-17, 1995

Including the World's Largest Commercial Exhibition of Related Equipment, Supplies, Software and Services

> MICROSCOPY SOCIETY OF AMERICA 53rd annual meeting THE HISTOCHEMICAL SOCIETY

> > **46TH ANNUAL MEETING**



SYMPOSIA AND CONTRIBUTED SESSIONS

▼Instrumentation & Methodologies

3-D Imaging & 3-D Reconstruction Advanced Computing in Microscopy Advances in Light Microscopy Auger Electron Spectroscopy **Biomaterials** Confocal Microscopy **Convergent Beam Diffraction** Correlative Microscopy (Tech Forum) Developments in Computer Controls Direct Digital Imaging & Microscope Automation Energy Loss & Filtering Spectroscopy **Field Emission** Image Formation & Recording Image Processing, Analysis, & Modeling Microbeam Mass Spectroscopy Near Field Microscopy **Optical & Electron Holography Optical Microspectroscopies** Scanning Probe Microscopy & Analysis SEM & TEM/STEM Surface Analysis Methods High-Res Intermediate- & High-Voltage EM in Biology & Materials Science Tomography X-ray EDS & XRF/XRD Techniques

SHORT COURSES

Immunocytochemistry & Protein Labeling: Ag-Enhanced Small Au Particles Approaches for *in situ* PCR & *in situ* Hybridization in Research & Diagnosis Cryotechniques for TEM, & Low-Temperature SEM Electron Diffraction in the TEM Introduction to Digital Imaging

▼Biological Sciences

Applied Biomedical Microscopies Cryotechniques Cytochemistry/Histochemistry EM Tomography in Biology Extracellular Matrix/Cell-ECM Interactions Functional Imaging of the Nervous System Functional Organization of the Cell Nucleus Histochemistry: Nucleic Acid Detection Immunology & Immunocytochemistry In Situ Hybridization Macromolecular Microscopy Membranes, Microdomains & Transport Microbiology **MRI** Microscopy Organelles, Chromosomes & Nuclei Pathology Phytomorphology & Phytobiology Reproduction & Developmental Biology Scanned Probe Microscopy

IN ADDITION

Over 130 Commercial Exhibits Over 600 Scientific Papers Over 50 Scientific Sessions Computer Software Exchange 8th Annual Golf Tournament Postage Stamp Exhibit 3rd Annual 5k Run/Walk Best Poster & Photomicrograph Awards Educational Outreach Program Public Education Panel Histochemical Society Lillie Awards MSA Presidential Student Awards EM Facilities Management (Tech Forum)

▼Physical Sciences

Amorphous/Disordered Materials Analytical Microscopy Advances: Ceramics Approaches to Catalyst Characterization Coatings **Electronic Materials** Geology/Mineralogy High Spatial Resolution Microanalysis & Microscopy In Situ Microscopy in Materials Research Magnetic Materials Microscopic Characterization of Materials Nano-Phase & Nano-Composite Materials **Oxidation & Corrosion** Petrology Phase Transformations Polymers, Metals & Alloys, Ceramics Quantitative Electron Diffraction Radiation-Sensitive Materials Small Particles/Clusters Surfaces & Interfaces Superconductors Tribology

TUTORIALS

Exploring Local Properties of Biological Surfaces with Atomic Force Microscopy Histochemical Methods for Localizing & Characterizing Glycoconjugates Energy Filtering in Biological EM Navigating the Internet Digital Imaging Electron Backscattered Diffraction: An Emerging Probe for Materials Characterization Atom Probe Analysis of the Solid–Liquid Interface Image Analysis Fundamentals

FOR MORE INFORMATION

Meeting Office ▼ P.O. Box EM ▼ Woods Hole, MA 02543 Toll-Free: 800-538-3672 ▼ Fax: 508-548-9053 ▼ E-mail: lmaser@mbl.edu